


# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm Breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

NOV 20 2009

Supervisor/Operator Performing the Verification Procedure:		DataMaster cdm S/N	130305 ✓
Name	Andre Achille	ID#	2385 Date 2-27-09 ✓
A	Agency	Bentley Police Dept	Phone # 907-543-3781
	Instrument Location	BPD SQUAD ROOM ✓	
B	Alco S/N	58427 ✓	Target Value .081 ✓
			High Pressure <del>0.08</del>
	Alco Test Values	1.084 ✓ 1 <sup>st</sup> Alco	1.085 ✓ 2 <sup>nd</sup> Alco
	Signature		
(OVER)			

(Do Not write in the area below)


BMB  
12/11/09

I, Nita J. Bolz, after being first duly sworn, depose and state as follows:


- (1) I am a Forensic Scientist IV at the State of Alaska Scientific Crime Detection Laboratory.
- (2) The Alaska Scientific Crime Detection Laboratory is an entity within the Department of Public Safety.
- (3) I am the Scientific Director of the State Breath Alcohol Program.
- (4) In that capacity, I am responsible for overseeing the breath alcohol program, including assuring that persons responsible for verifying the calibration of instruments are properly trained and qualified. I also am responsible for maintaining the records of the program.
- (5) The attached verification is a true and accurate verification of calibration that reflects a regularly conducted and regularly recorded activity of the breath alcohol program performed by a person trained and qualified to conduct the verification.
- (6) The referenced instrument is certified for evidentiary use in the State of Alaska.

  
Nita J. Bolz  
Scientific Director  
State Breath Alcohol Program

Subscribed and sworn before me this 10<sup>th</sup> day of Dec., 2009.

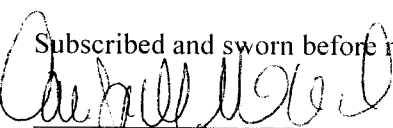 (Notary Seal Stamp)

Carolyn M. Noland  
Notary Public, State of Alaska  
Commission Expires with Office

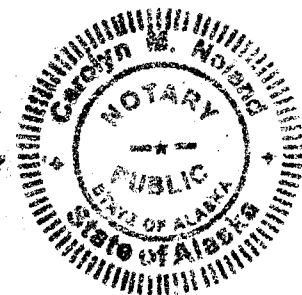

# VERIFICATION OF CALIBRATION REPORT

of DataMaster cdm breath Test Instrument

State of Alaska

Scientific Crime Detection Laboratory - Statewide Breath Alcohol Program

DataMaster cdm S/N 130305

(CONTINUED FROM FRONT PAGE)

C

TAPE THE TEST STRIP FROM THE NONDRINKING SUBJECT TEST AND THE DIAGNOSTIC CHECK IN THE MARKED BOXES.

## NONDRINKING SUBJECT TEST

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 170305

FEBRUARY 27, 2009

OPERATOR'S NAME:

ADREE ADREE

OPERATOR'S NUMBER: 2385

SUBJECT'S LAST NAME:

TEST

SUBJECT'S FIRST NAME/MI :

VOC

S/L #: 1234567

DEPT/AGENCY: BET1

LABE REPORT: 09-012709

TEST TYPE: T

ALCO TARGET VALUE: .081

ALCO S/N: 58427

--- BREATH ANALYSIS ---

.081 ADJUSTED FOR 30.17 in

ALCO TARGET .081 16:37

BLANK TEST .000 16:38

INTERNAL STANDARD VERIFIED 16:38

ALCO TO 30.17 in .084 16:39

BLANK TEST .000 16:40

SUBJECT SAMPLE .000 16:40

BLANK TEST .000 16:41

ALCO TO 30.17 in .085 16:41

BLANK TEST .000 16:42

## DIAGNOSTIC CHECK

ALASKA DEPARTMENT OF PUBLIC SAFETY  
DATAMASTER cdm 170305

FEBRUARY 27, 2009

TIME 16:32

--- DIAGNOSTIC CHECK ---

COMPUTER: OKAY

PROGRAM: OKAY

SOFTWARE DATE: 02/20/01

HEATERS

SAMPLE CHAMBER: 48c

BREATH TUBE: 41c

BAROMETER: 30.17 in

FLOW DETECTOR: OKAY

PUMP

HIGH SPEED: OKAY

DETECTOR: OKAY

FILTERS: OKAY

QUARTZ STANDARD: OKAY

CALIBRATION: OKAY

PRINTER TEST

!""%&'()\*+,-./0123456789:;<=>?@ABCDEFB  
HIJKLMNPQRSTUWXYZ[\]^\_`abcedefghijklmnop  
qrstuvwxyz{|}~